

EU Quality Management System Certificate

Regulation (EU) 2017/745, Annex IX Chapter I and III

MDR 724378 R000

Manufacturer: Enztec Limited

Address:

3/17 Print Place
Middleton
Christchurch
8024
New Zealand

Single Registration Number: Not Available

EU Authorised Representative: Advena Limited

Address:

Tower Business Centre, 2nd Flr.,
Tower Street
Swatar, BKR 4013
Malta

Scope: See attached **Device Schedule**

On the basis of our examination of the quality system in accordance with Regulation (EU) 2017/745, Annex IX Chapter I and III, the quality system meets the requirements of the Regulation. For the placing on the market of Class III and Class IIb implantable devices an Annex IX Chapter II certificate is required.

For and on behalf of BSI, a Notified Body for the above Regulation (Notified Body Number 2797):



Gary E Slack, Senior Vice President Medical Devices

First Issued: **2020-08-06**

Date: **2020-10-19**

Expiry Date: **2025-08-05**

...making excellence a habit.™

Page 1 of 3

Validity of this certificate is conditional on the Manufacturer's quality system being maintained to the requirements of the Regulation as demonstrated through the required surveillance activities of the Notified Body.
This certificate was issued electronically and is bound by the conditions of the contract.

EU Quality Management System Certificate

Regulation (EU) 2017/745, Annex IX Chapter I and III


MDR 724378 R000

Device Schedule: Class IIa, Custom-made and other devices

| Device(s) | Risk Classification |
|---|---------------------|
| Orthopaedic instruments connected to an active device - Reusable Surgical Instruments | Class IIa |
| Reusable surgical instruments "Orthopaedic instruments" | Class Ir |
| Reusable surgical instruments "Orthopaedic instruments" | Class Ir & Im |

For Class Im devices, the Notified Body conformity assessment is limited to the aspects relating to the conformity of the devices with the metrological requirements.

For Class Ir devices (Class I re-usable surgical instruments), the Notified Body conformity assessment is limited to the aspects relating to the reuse of the device.

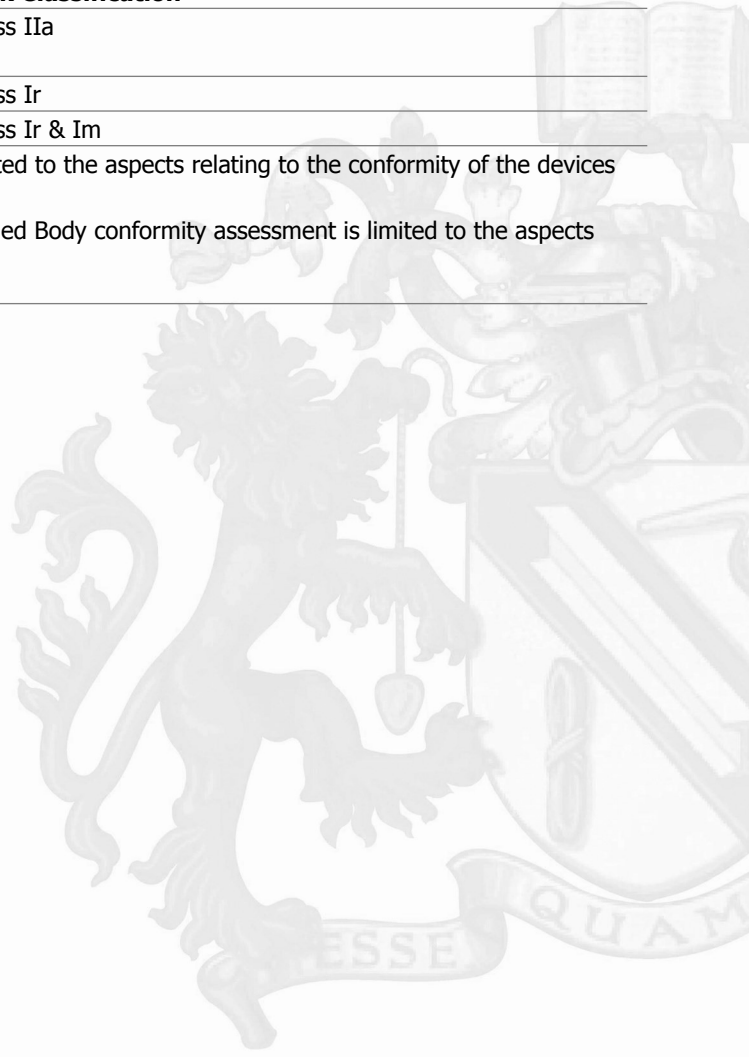

First Issued: **2020-08-06**

Date: **2020-10-19**

Expiry Date: **2025-08-05**

...making excellence a habit.™

Validity of this certificate is conditional on the Manufacturer's quality system being maintained to the requirements of the Regulation as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.

EU Quality Management System Certificate


Regulation (EU) 2017/745, Annex IX Chapter I and III

MDR 724378 R000

Certificate History

(References to applicable Common Specifications, Harmonized Standards complied with, and the relevant test and audit reports that support any of the below certificate changes may be requested from Certificate.Verification@bsigroup.com)

| Date | Reference number | Action |
|----------------|------------------|--|
| 06 August 2020 | 3147250 | First Issue |
| Current | 3312997 | Add Class IIa Instrument attached to an active device, to schedule |

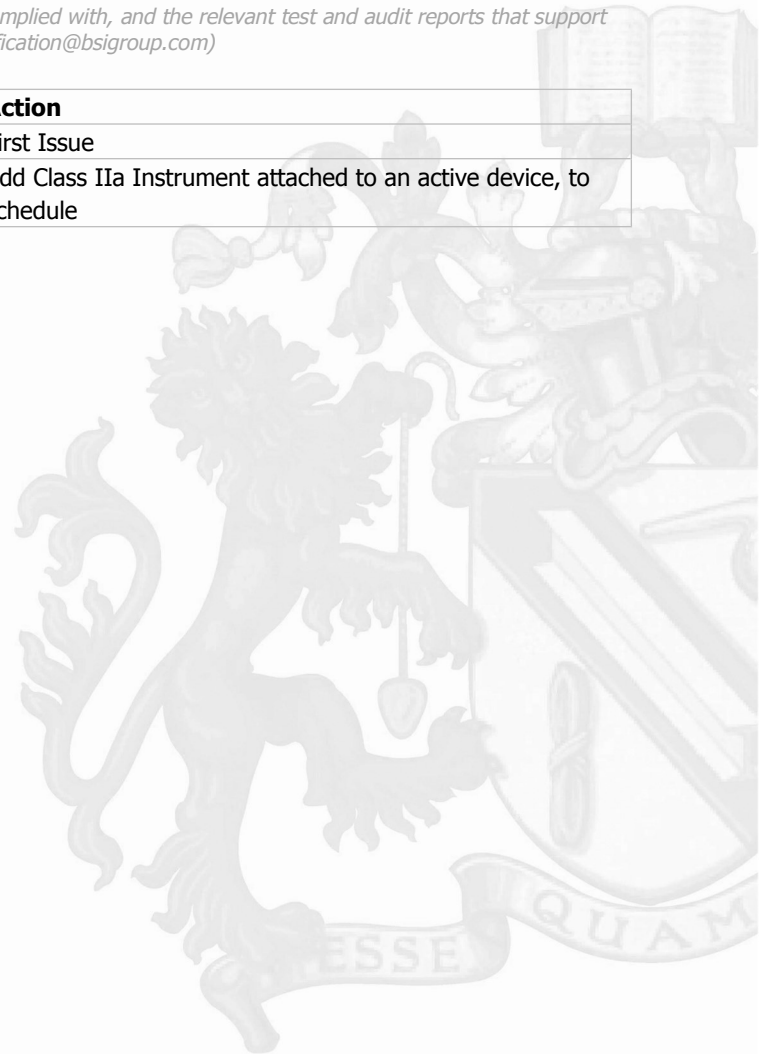

First Issued: **2020-08-06**

Date: **2020-10-19**

Expiry Date: **2025-08-05**

...making excellence a habit.™

Page 3 of 3

Validity of this certificate is conditional on the Manufacturer's quality system being maintained to the requirements of the Regulation as demonstrated through the required surveillance activities of the Notified Body.

This certificate was issued electronically and is bound by the conditions of the contract.